

Available in Platinum and CERECYTE®



CASHMERE™

microcoil

14

COMPLEX STRETCH-RESISTANT (SRC14)

CATALOG NUMBER	LOOP DIAMETER	OVERALL LENGTH
SRC140225-20	2 mm	2.5 cm
SRC140303-20	3 mm	3 cm
SRC140304-20	3 mm	4 cm
SRC140306-20	3 mm	6 cm
SRC140445-20	4 mm	4.5 cm
SRC140406-20	4 mm	6 cm
SRC140408-20	4 mm	8 cm
SRC140507-20	5 mm	7 cm
SRC140512-20	5 mm	12 cm
SRC140609-20	6 mm	9 cm
SRC140615-20	6 mm	15 cm
SRC140711-20	7 mm	11 cm
SRC140717-20	7 mm	17 cm
SRC140812-20	8 mm	12 cm
SRC140820-20	8 mm	20 cm
SRC140914-20	9 mm	14 cm
SRC140922-20	9 mm	22 cm
SRC141016-20	10 mm	16 cm
SRC141025-20	10 mm	25 cm
SRC141118-20	11 mm	18 cm
SRC141127-20	11 mm	27 cm
SRC141219-20	12 mm	19 cm
SRC141230-20	12 mm	30 cm

COMPLEX CERECYTE (CRC14)

CATALOG NUMBER	LOOP DIAMETER	OVERALL LENGTH
CRC140225-30	2 mm	2.5 cm
CRC140303-30	3 mm	3 cm
CRC140304-30	3 mm	4 cm
CRC140306-30	3 mm	6 cm
CRC140445-30	4 mm	4.5 cm
CRC140406-30	4 mm	6 cm
CRC140408-30	4 mm	8 cm
CRC140507-30	5 mm	7 cm
CRC140512-30	5 mm	12 cm
CRC140609-30	6 mm	9 cm
CRC140615-30	6 mm	15 cm
CRC140711-30	7 mm	11 cm
CRC140717-30	7 mm	17 cm
CRC140812-30	8 mm	12 cm
CRC140820-30	8 mm	20 cm
CRC140914-30	9 mm	14 cm
CRC140922-30	9 mm	22 cm
CRC141016-30	10 mm	16 cm
CRC141025-30	10 mm	25 cm
CRC141118-30	11 mm	18 cm
CRC141127-30	11 mm	27 cm
CRC141219-30	12 mm	19 cm
CRC141230-30	12 mm	30 cm



821 Fox Lane
San Jose, CA 95131
United States
T 408.433.1400
F 408.433.1401

Avenue des Baumettes 7
1020 Renens
Switzerland
T +41.21.631.3434
F +41.21.631.3444

1st Floor, Unit 4
Stansted Courtyard
Takeley
Bishop's Stortford
Essex
CM22 6PU
United Kingdom
T +44.800.612.6363
F +44.800.612.8484


Cerecyte® Coils



IT'S INSIDE™

CAUTION: Federal (U.S.A.) law restricts this device to sale by or on the order of a physician.
MICRUS, CERECYTE, and the M logo are registered trademarks of Micrus Endovascular Corporation. CASHMERE, IT'S INSIDE, and the purple coil logo are trademarks of Micrus Endovascular Corporation. Other product names or marks are the property of their respective owners.
© 2008 Micrus Endovascular Corporation. All rights reserved.

P/N 50764-01 REV C

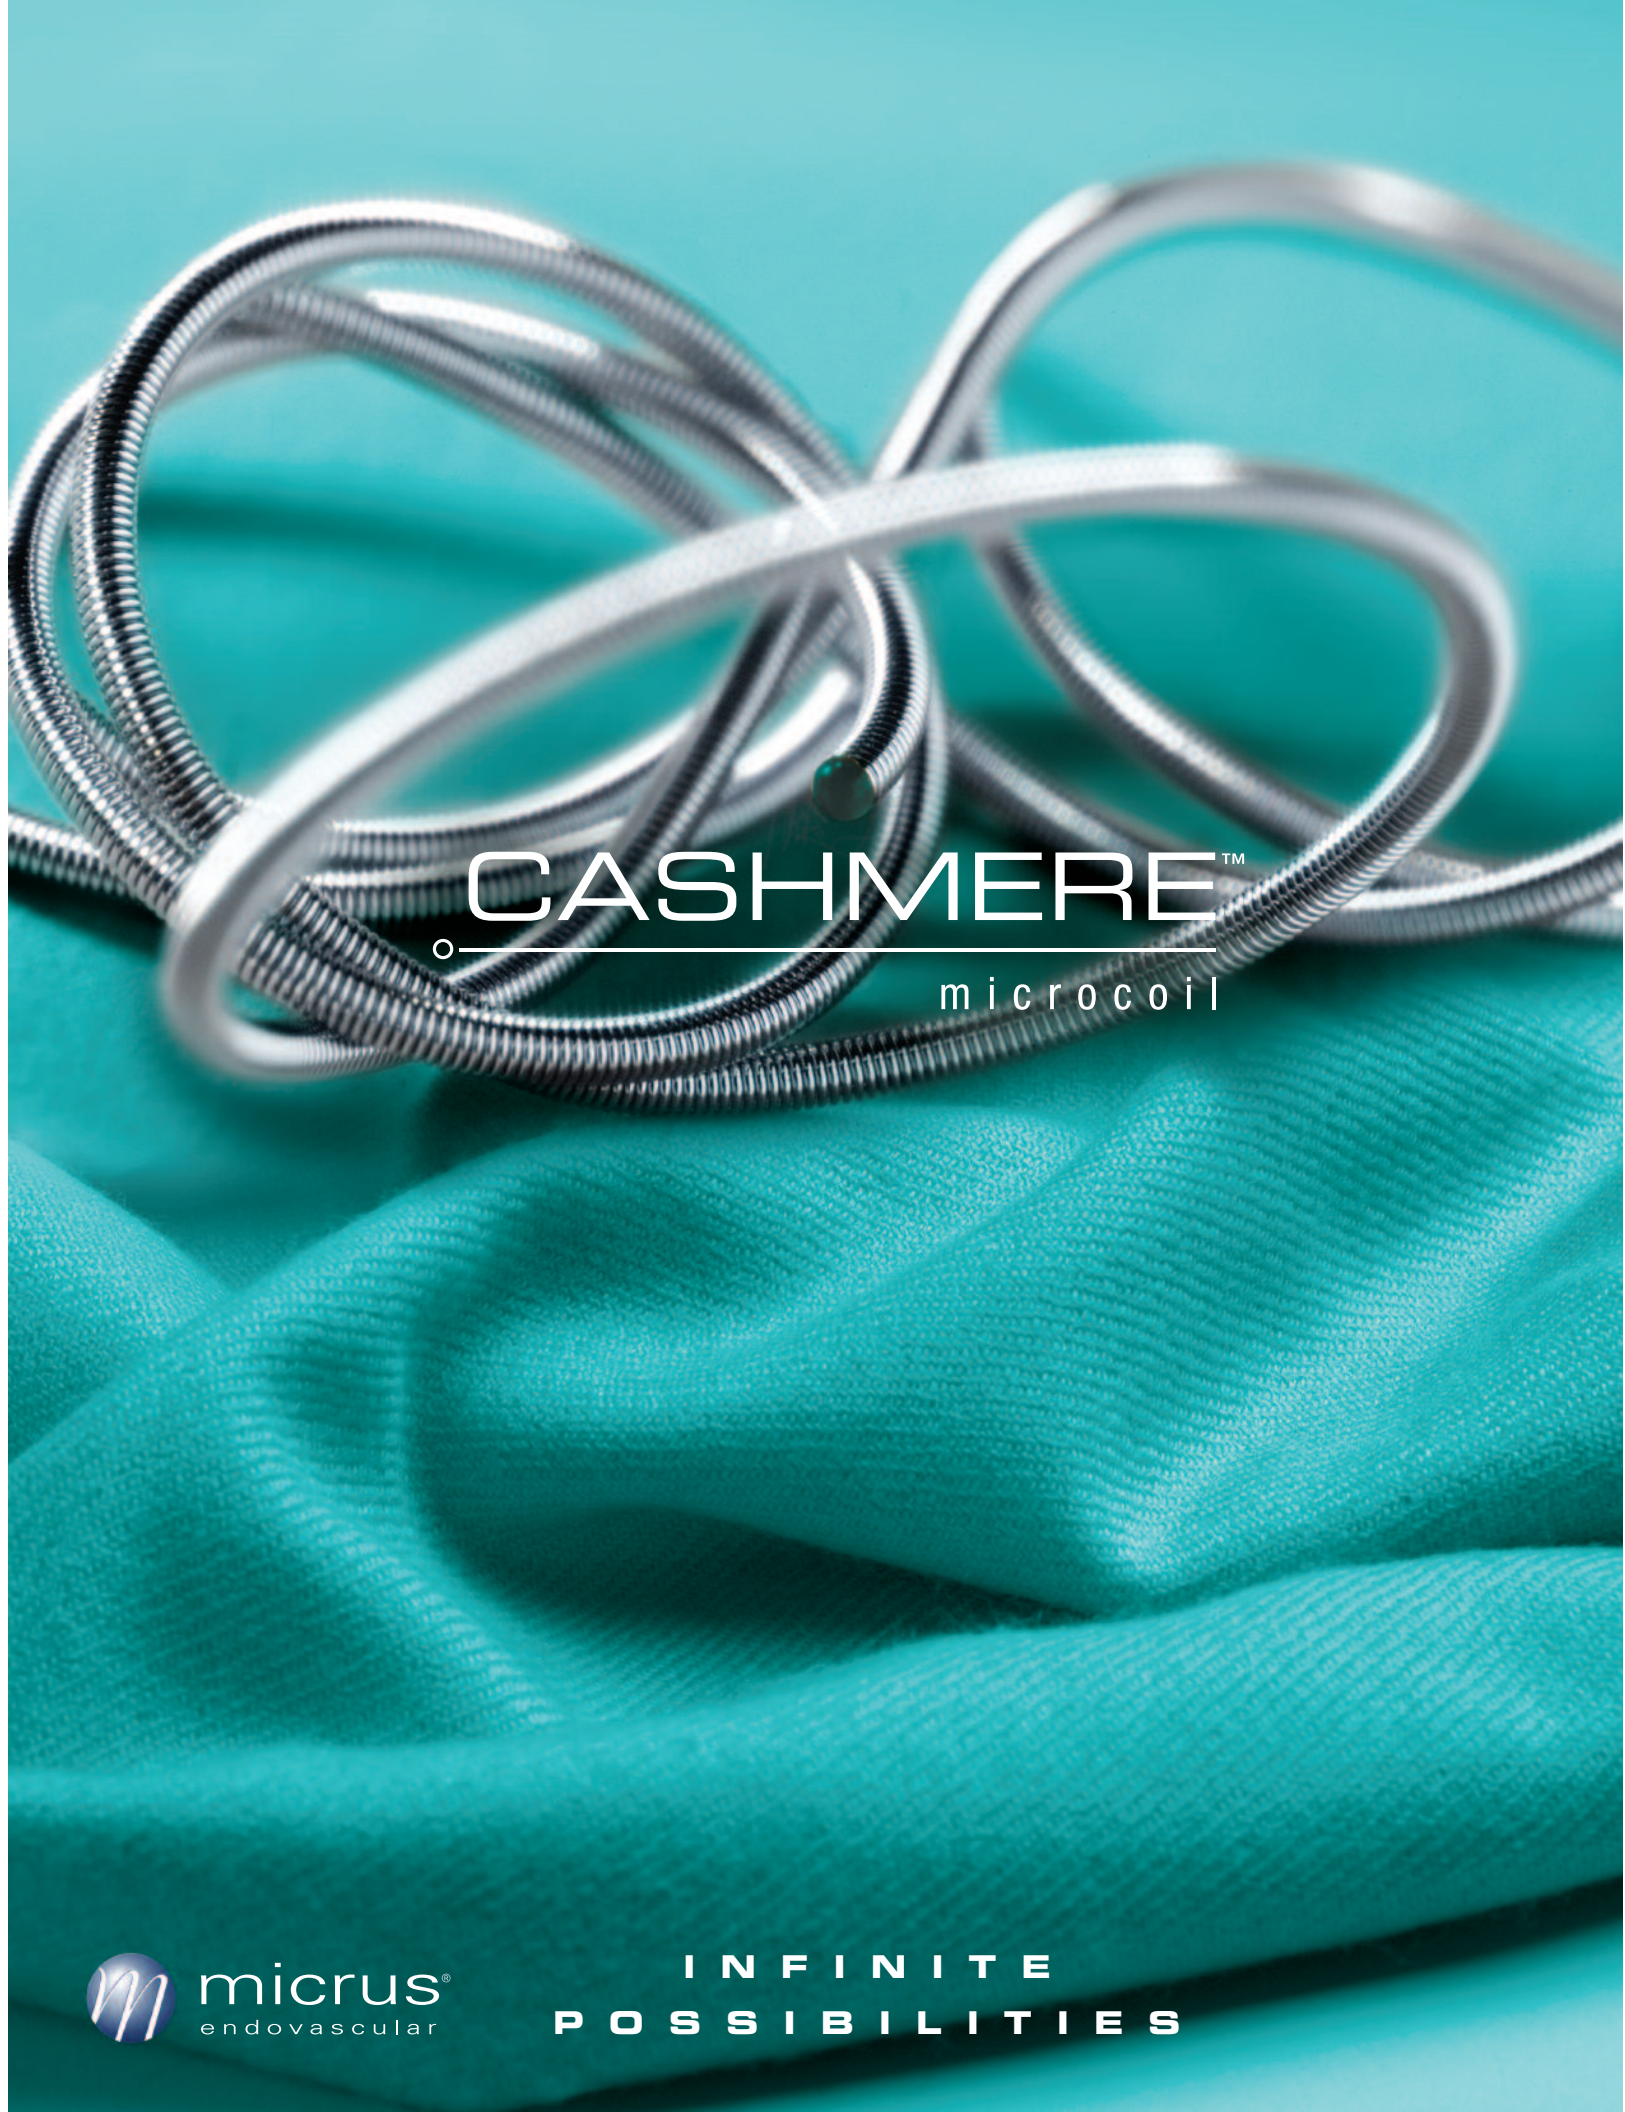

INFINITE
POSSIBILITIES



The Feeling of Infinity

The CASHMERE™ Microcoil is a breakthrough in softness and conformability designed for framing and filling an infinite array of aneurysm shapes. The unique, complex design combines helical and Infinity loops, allowing the CASHMERE Microcoil to comply with the walls of the aneurysm while remaining clear of the parent vessel. Combine this with increased packing volume through your frontline microcatheter* and get a world of infinite possibilities.



∞ Conformability

Novel, complex shape designed for conformability.

- Infinity loops seek out and respect aneurysm periphery even in complex shapes
- Two initial helical loops help anchor the coil within the aneurysm
- Stretch-resistant member provides increased safety and positioning options allowing for coil repositioning

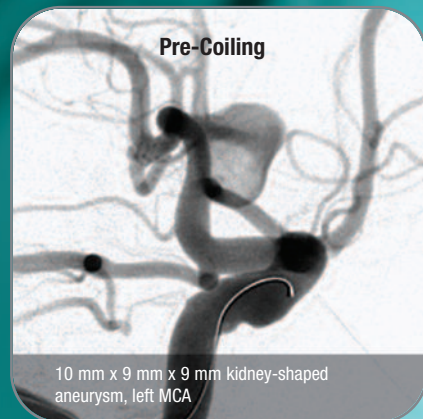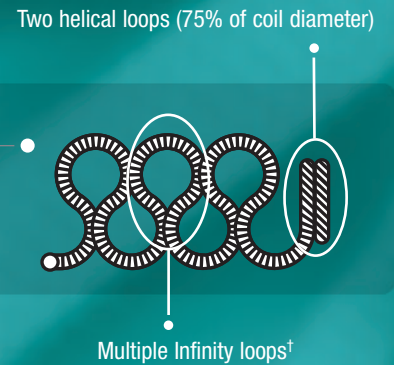

Images courtesy of Dr. Ajay Wakhloo, University of Massachusetts

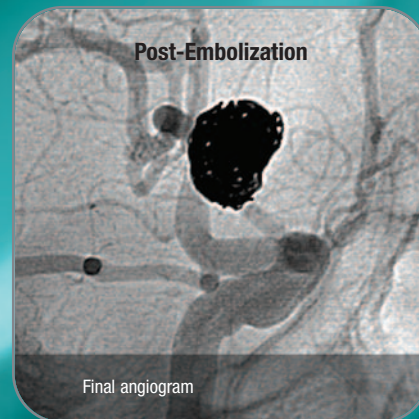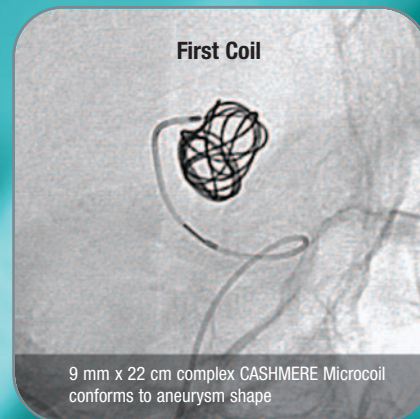


Designed for an infinite array of aneurysm shapes

∞ Softness

New proprietary wind provides increased coil softness.


- Appropriate for both ruptured and unruptured aneurysms
- Allows for accurate coil sizing to the aneurysm
- Softness comparable to the Cordis® Orbit™ Complex Fill‡
- Softer than leading 10 System microcoils, including the Boston Scientific GDC® 360° Soft SR†
- The 2mm-4mm Cashmere Microcoils were designed with even greater softness; over 50% softer than the 5mm-12mm sizes

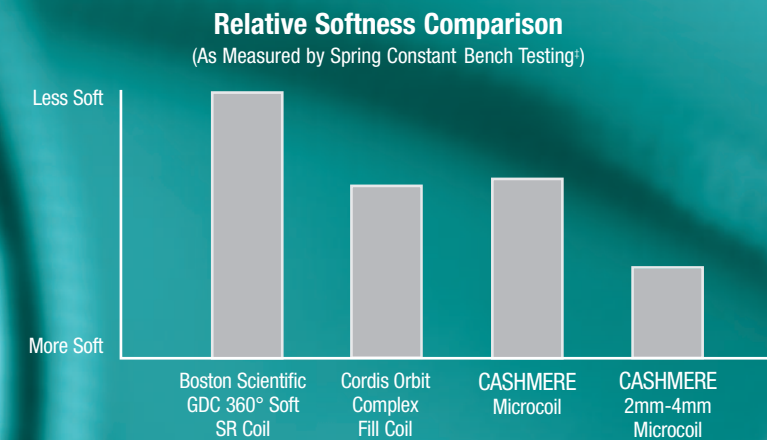

∞ Performance

Increased packing volume through frontline microcatheters.

- Compatible with 14 System microcatheters with IDs ranging from .0165" to .019"
- More packing volume per cm than 10 and 12 System microcoils‡
- Provides enhanced coil radiopacity compared with smaller system microcoils

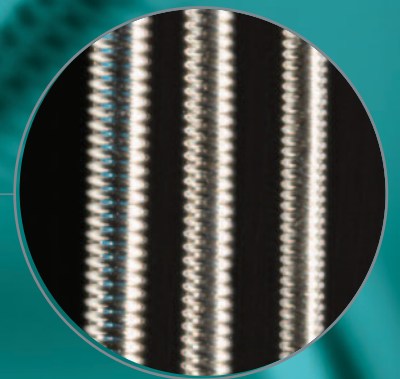

14 System CASHMERE, 12 System, and 10 System microcoil segments

∞ CERECYTE®: The Inside Advantage

CERECYTE Coil PGA member **inside** the coil.

- Bare platinum handling characteristics
- Induced tissue response§
- Stretch-resistant
- Maintains overall platinum volume after polymer has been absorbed

* Compatible with microcatheters with inner diameters ranging from .0165" to .019".
 † Total number of Infinity loops is determined by overall coil length.
 ‡ Data on file, Micrus Endovascular Corporation.
 § Polyglycolic acid appears to have induced tissue response. Animal studies data on file, Micrus Endovascular Corporation.